



Tone 01

- ① lab(80.4, 6.5, 11.9)
- ② lab(78.7, 10.2, 12.0)
- ③ lab(77.2, 12.1, 13.9)
- ④ lab(75.3, 13.5, 13.6)
- ⑤ lab(70.2, 14.6, 18.4)

CIELAB values measured for D50 reference

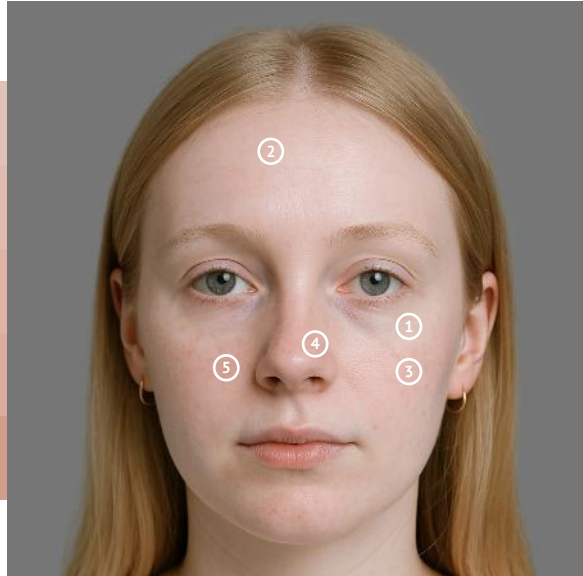

Spot Measurement Reflectance Spectra

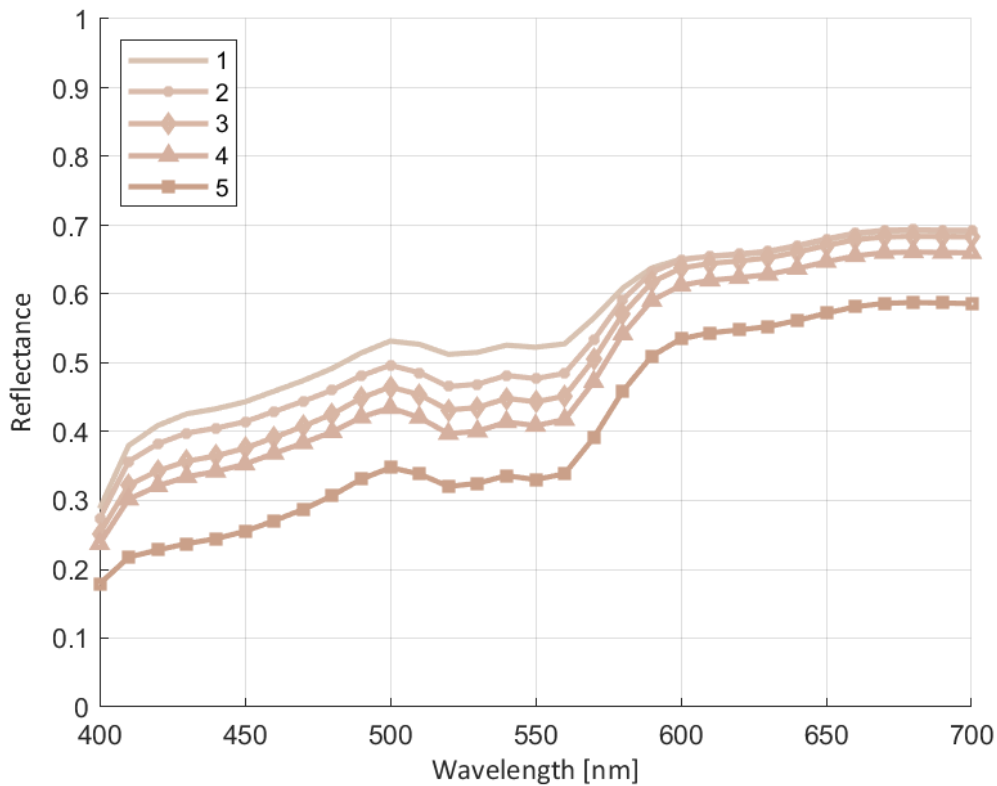

Tone 02

① lab(77.2, 11.8, 15.6)


② lab(75.5, 12.2, 16.2)

③ lab(75.8, 12.5, 18.2)


④ lab(72.4, 14.0, 20.0)

⑤ lab(68.5, 16.0, 19.1)

CIELAB values measured for D50 reference

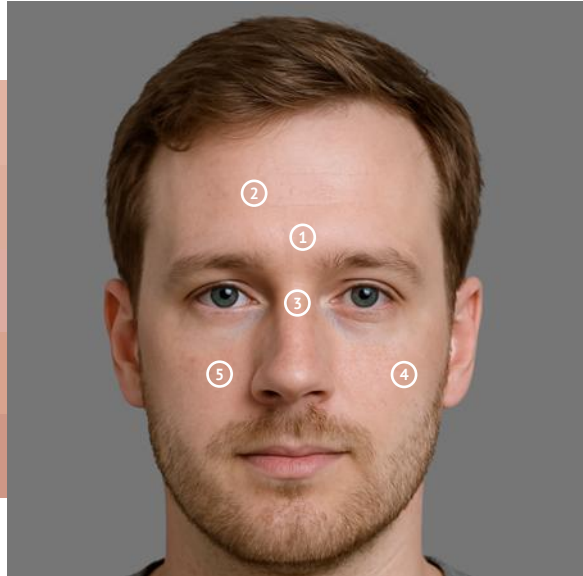


Spot Measurement Reflectance Spectra

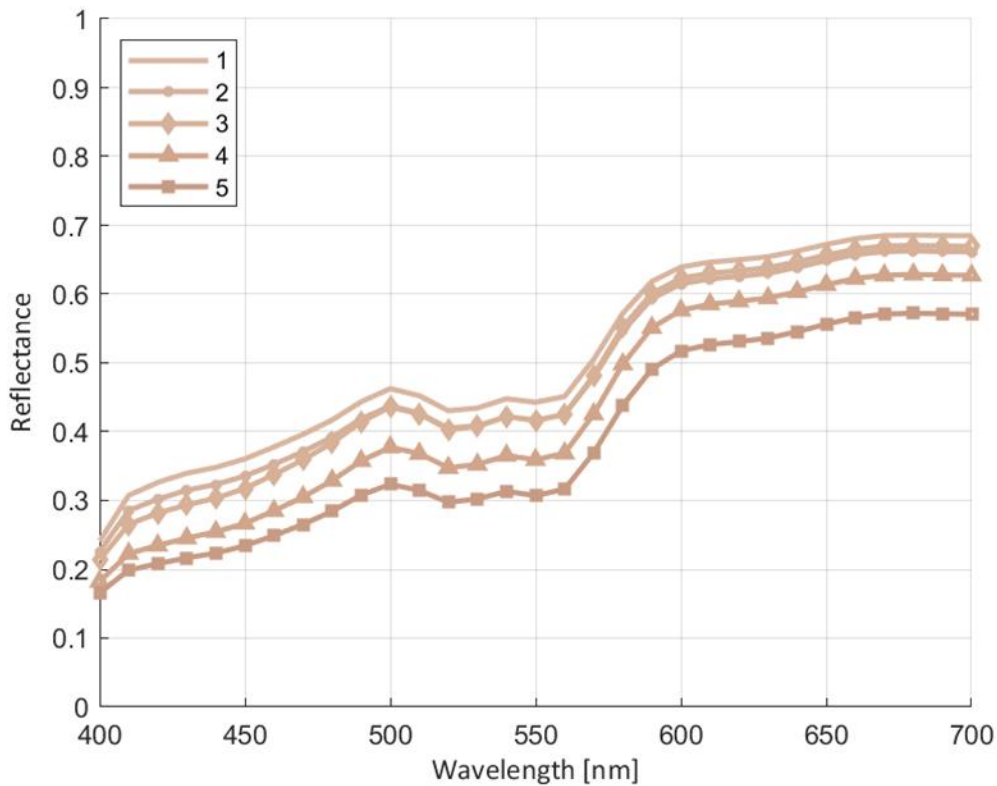


Tone 03

- ① lab(72.2, 11.6, 16.9)
- ② lab(71.5, 11.4, 20.2)
- ③ lab(69.3, 12.1, 22.6)
- ④ lab(66.3, 13.0, 22.5)
- ⑤ lab(62.0, 15.0, 21.7)

CIELAB values measured for D50 reference

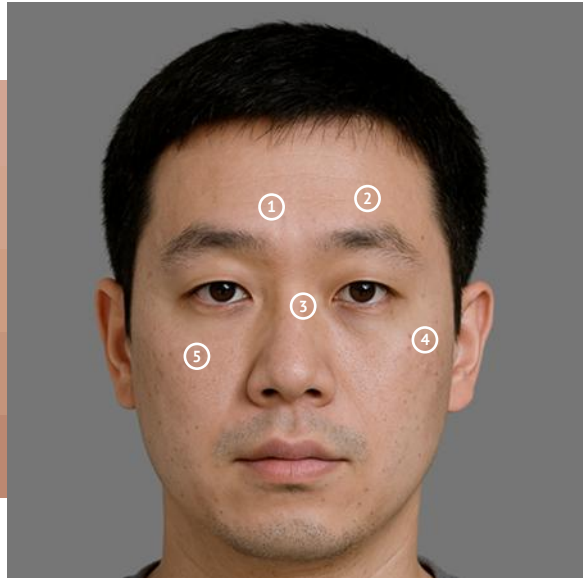

Spot Measurement Reflectance Spectra

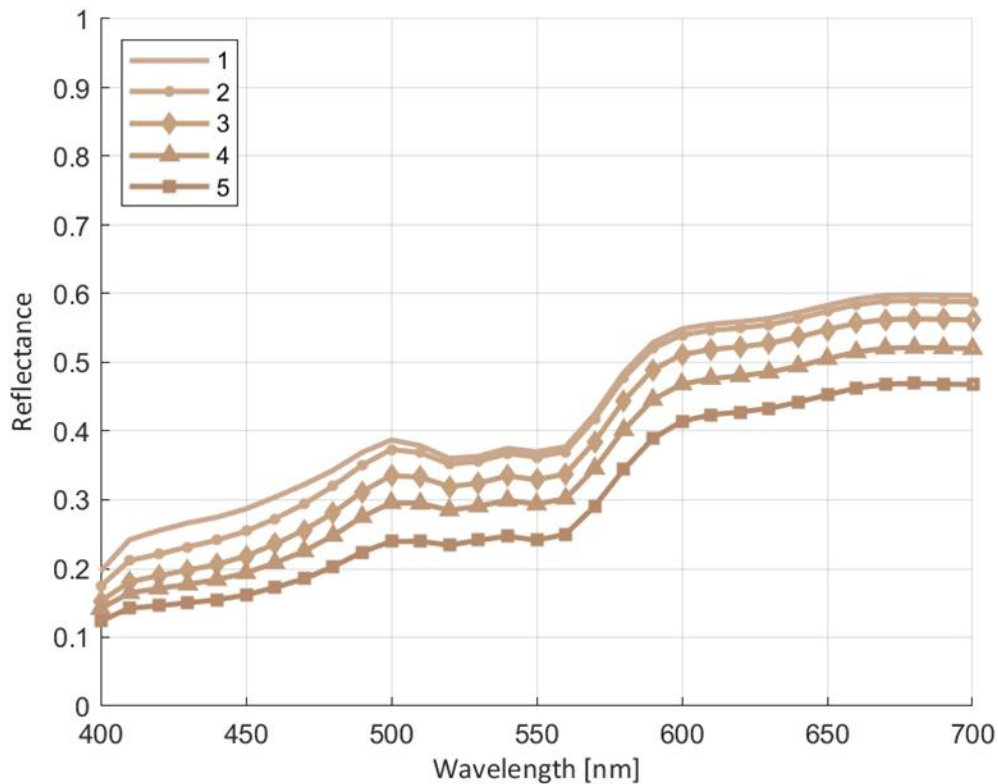

Tone 04

① lab(65.9, 14.1, 22.9)


② lab(63.2, 17.2, 22.8)

③ lab(58.3, 15.5, 24.3)


④ lab(56.1, 14.9, 25.1)

⑤ lab(50.2, 16.5, 24.5)

CIELAB values measured for D50 reference

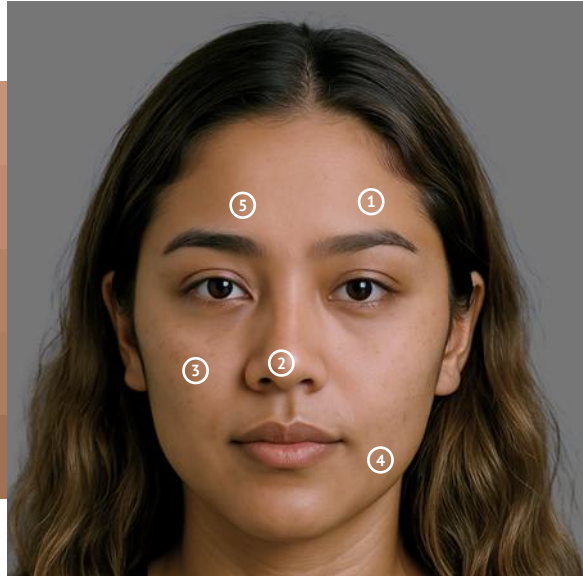

Spot Measurement Reflectance Spectra

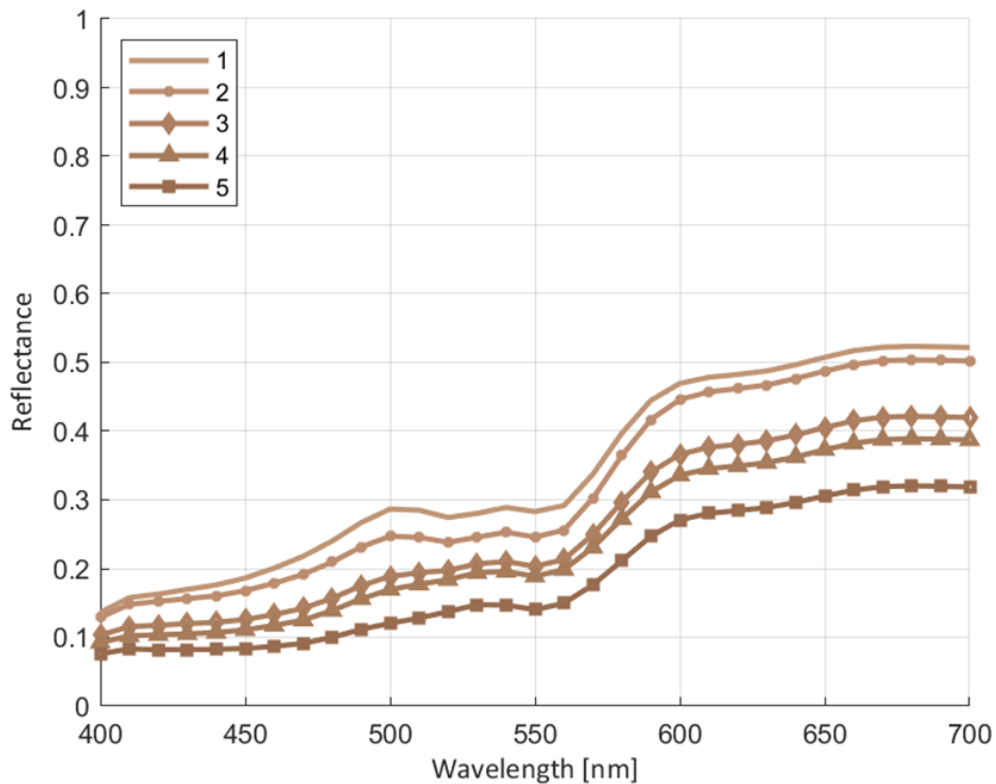

Tone 05

① lab(58.5, 16.2, 22.7)


② lab(56.1, 17.9, 23.0)

③ lab(53.7, 17.9, 23.4)


④ lab(51.9, 18.3, 22.5)

⑤ lab(48.6, 18.7, 22.0)

CIELAB values measured for D50 reference

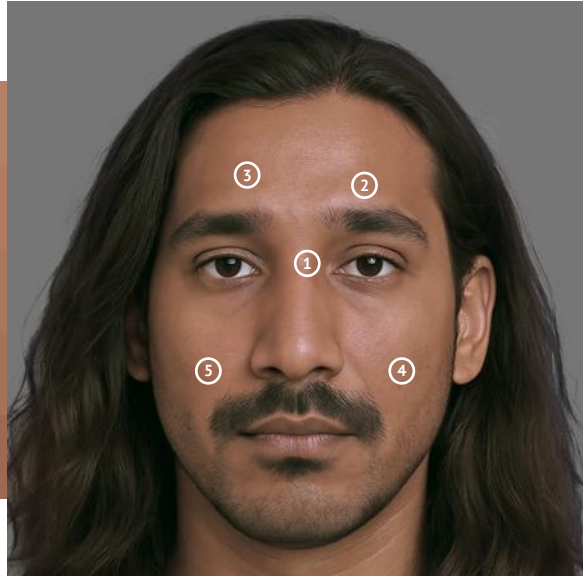

Spot Measurement Reflectance Spectra

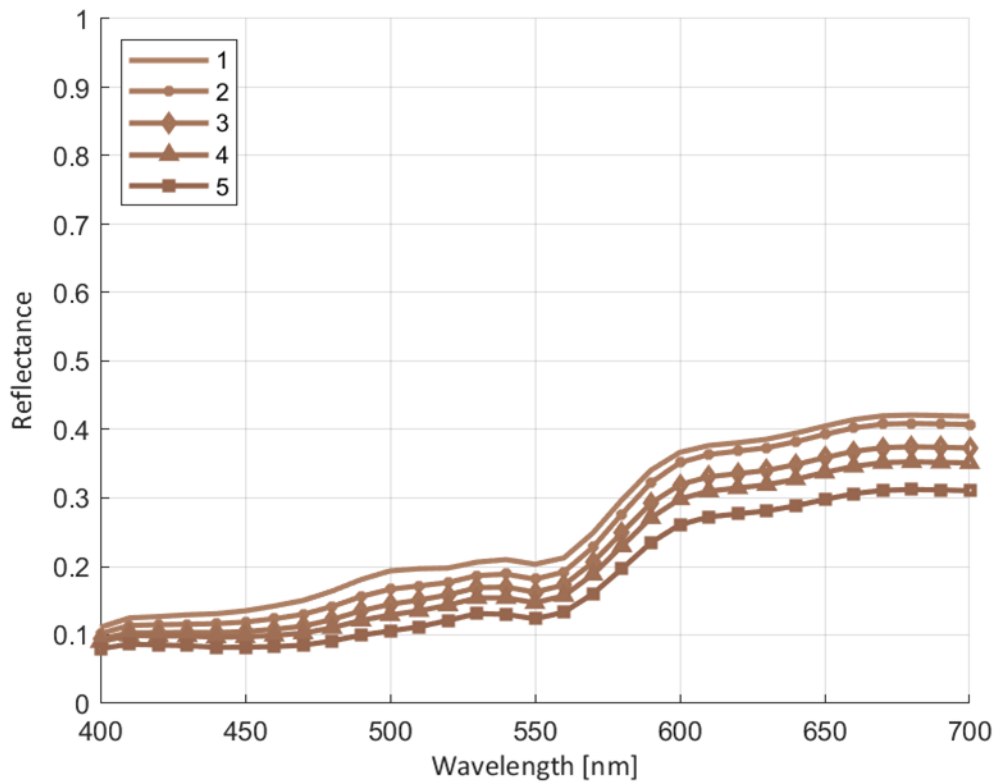

Tone 06

① lab(57.4, 20.8, 22.6)


② lab(56.5, 19.2, 22.3)

③ lab(55.3, 19.5, 20.9)


④ lab(54.3, 19.5, 22.6)

⑤ lab(49.7, 20.6, 20.6)

CIELAB values measured for D50 reference

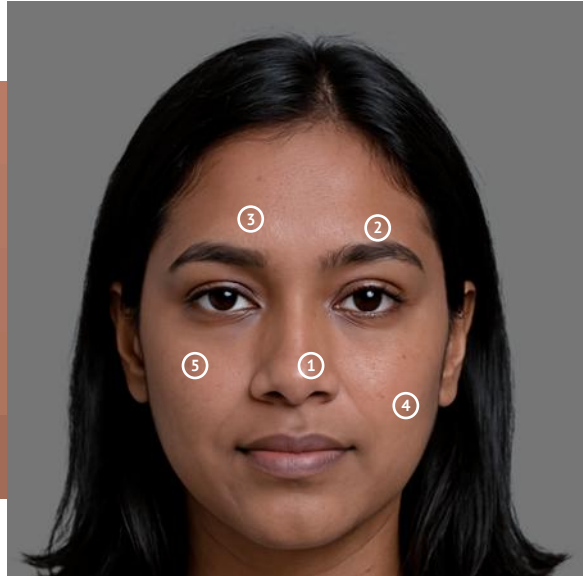

Spot Measurement Reflectance Spectra

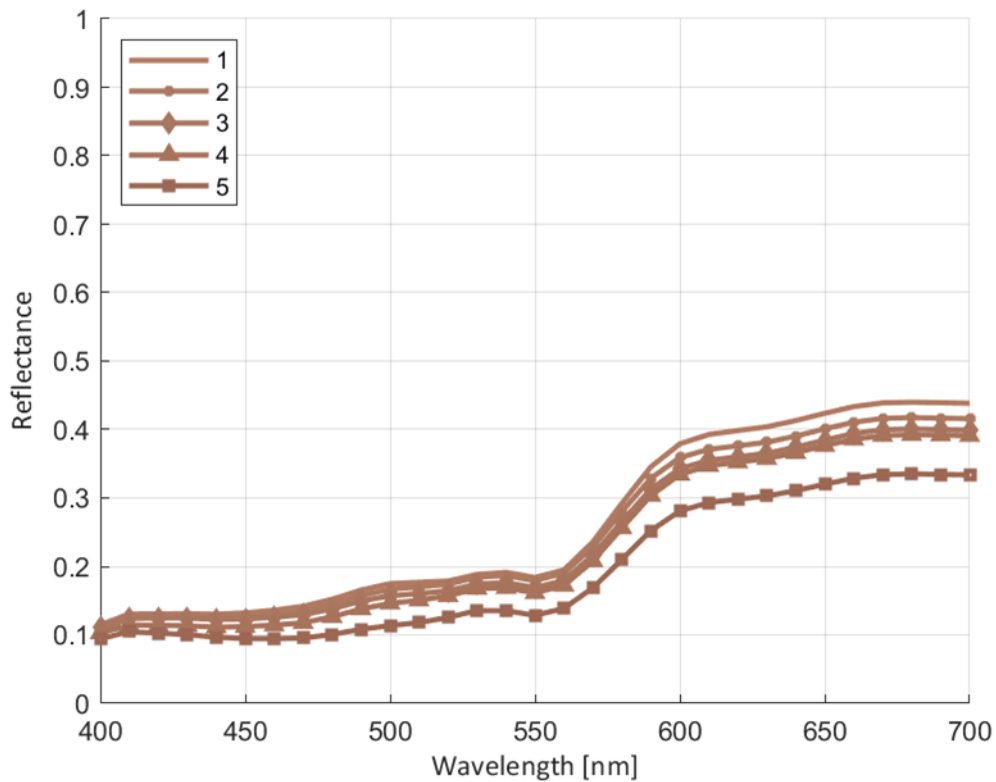

Tone 07

① lab(50.1, 18.5, 24.1)


② lab(46.0, 18.8, 24.1)

③ lab(41.1, 18.3, 22.7)


④ lab(39.7, 18.7, 22.0)

⑤ lab(38.2, 17.2, 21.9)

CIELAB values measured for D50 reference

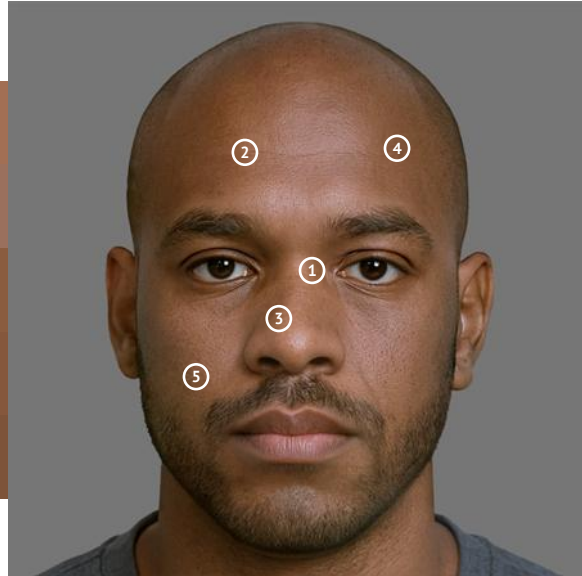

Spot Measurement Reflectance Spectra

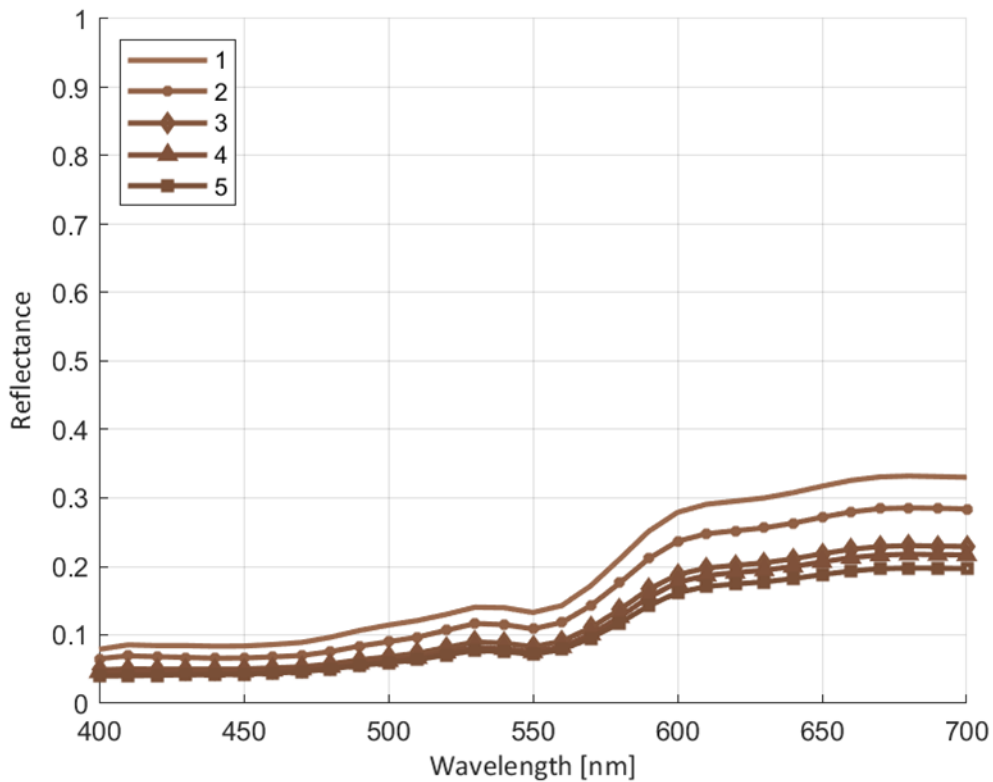

Tone 08

① lab(45.7, 19.9, 23.4)


② lab(42.3, 19.7, 23.0)

③ lab(38.1, 20.2, 23.1)


④ lab(35.9, 18.3, 19.3)

⑤ lab(34.7, 17.7, 19.0)

CIELAB values measured for D50 reference

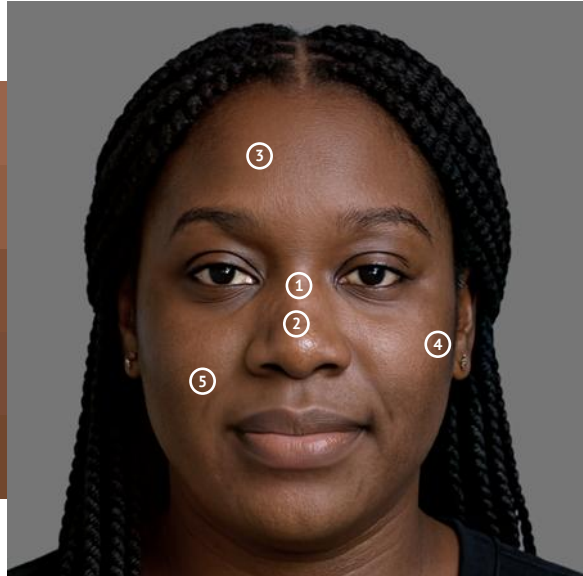

Spot Measurement Reflectance Spectra

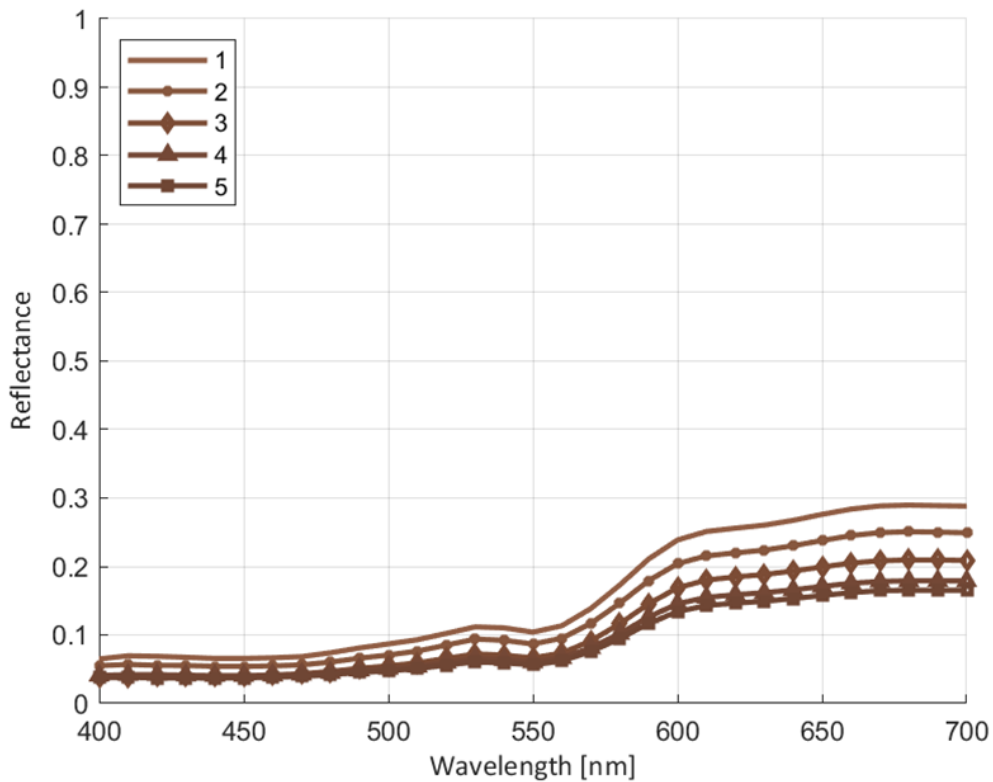

Tone 09

① lab(44.8, 16.7, 22.9)


② lab(42.7, 15.1, 20.4)

③ lab(37.9, 13.7, 18.1)


④ lab(33.8, 12.8, 15.9)

⑤ lab(28.8, 10.8, 11.8)

CIELAB values measured for D50 reference

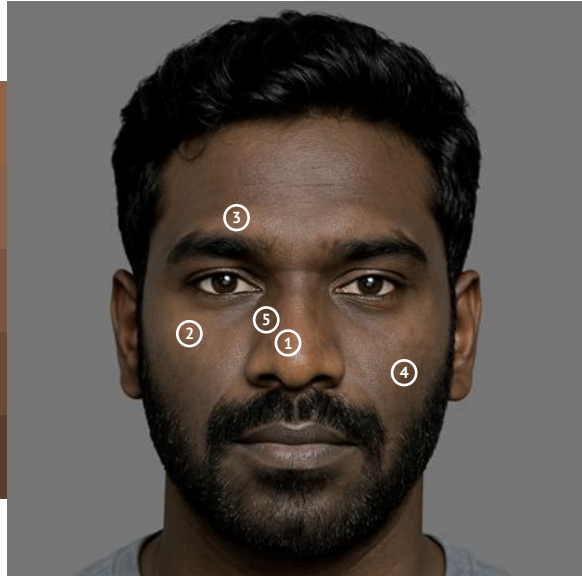

Spot Measurement Reflectance Spectra

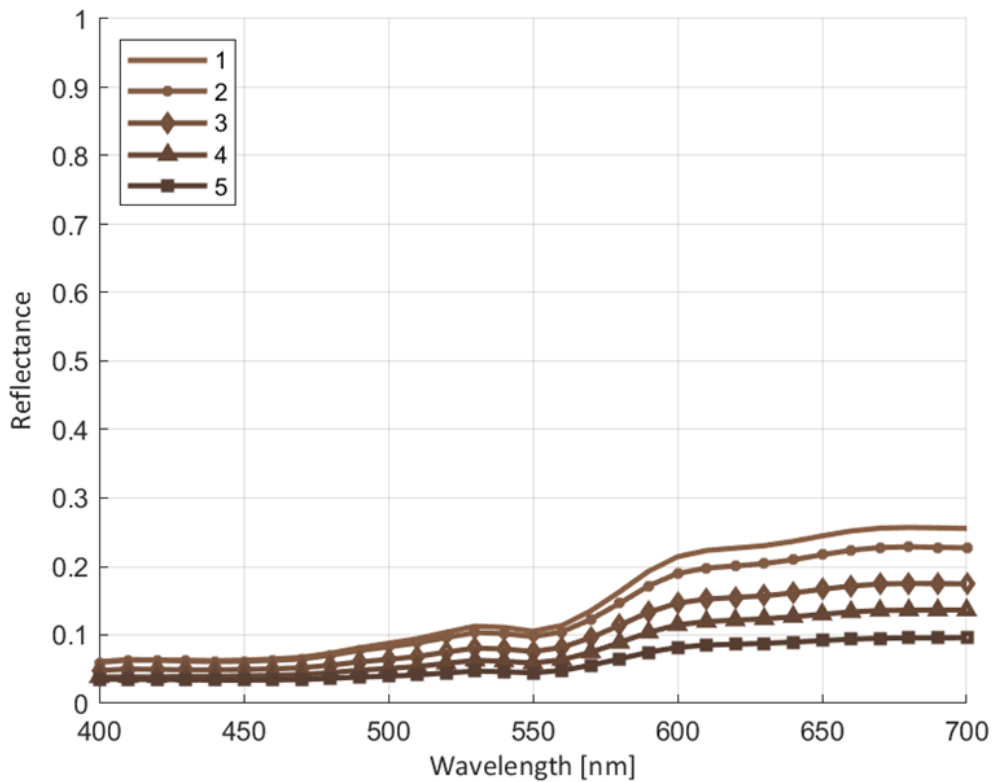

Tone 10

① lab(29.3, 9.41, 10.4)


② lab(29.1, 9.96, 12.1)

③ lab(25.8, 8.66, 8.96)

④ lab(25.0, 8.29, 8.23)

⑤ lab(23.7, 7.81, 7.18)

CIELAB values measured for D50 reference

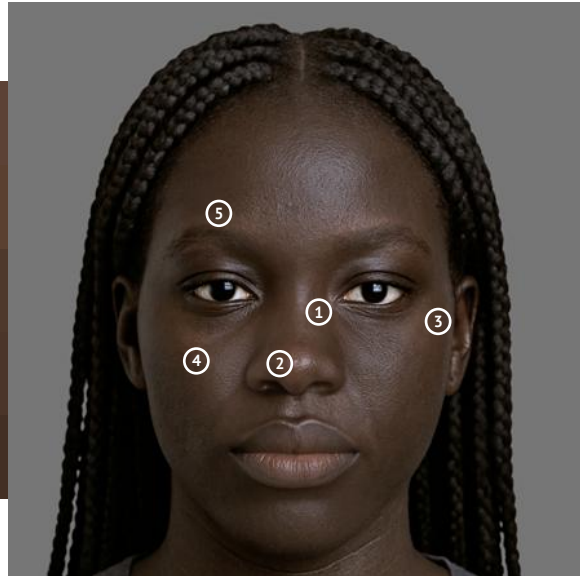

Spot Measurement Reflectance Spectra

